




1 & 3 AMP STANDARD

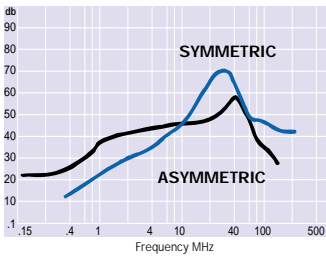


6 & 10 AMP STANDARD

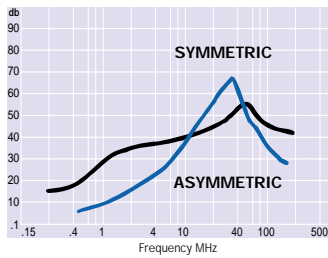

1 & 3 AMP MEDICAL

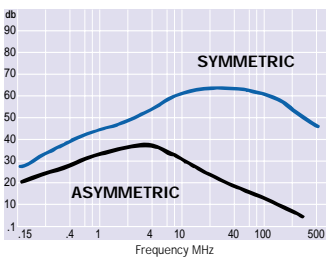

6 & 10 AMP MEDICAL

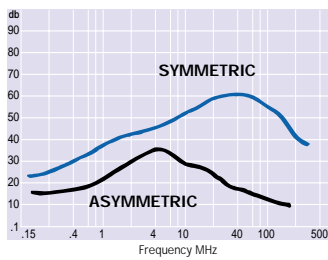

SF 1050	Rated Current A	Leakage Current @ 250V 50Hz	Inductance mH	Connections Input	Output	Resistor Value MΩ	Approvals			
Standard Version										
SF 1050-1/01	1	0.2mA max	3.0	IEC 320	6.3 x 0.8 Faston	Not Fitted	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
SF 1050-3/01	3	0.2mA max	0.85	IEC 320	6.3 x 0.8 Faston	Not Fitted	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
SF 1050-6/01	6	0.2mA max	0.35	IEC 320	6.3 x 0.8 Faston	Not Fitted	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
SF 1050-10/01	10	0.2mA max	0.16	IEC 320	6.3 x 0.8 Faston	Not Fitted	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
Medical Version										
SF 1050M-1/01	1	5µA max	3.0	IEC 320	6.3 x 0.8 Faston	1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
SF 1050M-3/01	3	5µA max	0.85	IEC 320	6.3 x 0.8 Faston	1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
SF 1050M-6/01	6	5µA max	0.35	IEC 320	6.3 x 0.8 Faston	1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
SF 1050M-10/01	10	5µA max	0.16	IEC 320	6.3 x 0.8 Faston	1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	


Temperature Range: -25°C to +85°C
Operating Voltage: 250Vac
Operating Frequency: 0 to 400Hz
Test Voltage: L+N to ground, 2700Vdc, 2 seconds

Approved
 Submitted for Approval

IEC 950 (EN 60950 Applications)


DIMENSIONS

All dimensions are nominal and in mm

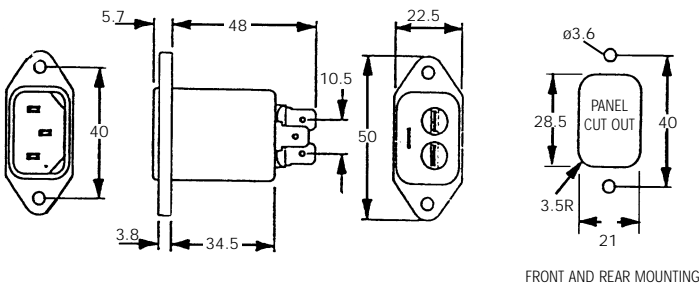

CIRCUIT DIAGRAMS

Standard Version

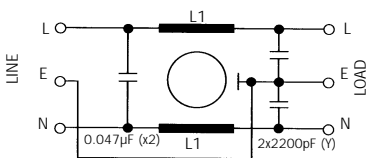

Medical Version (Suffix 'M')

